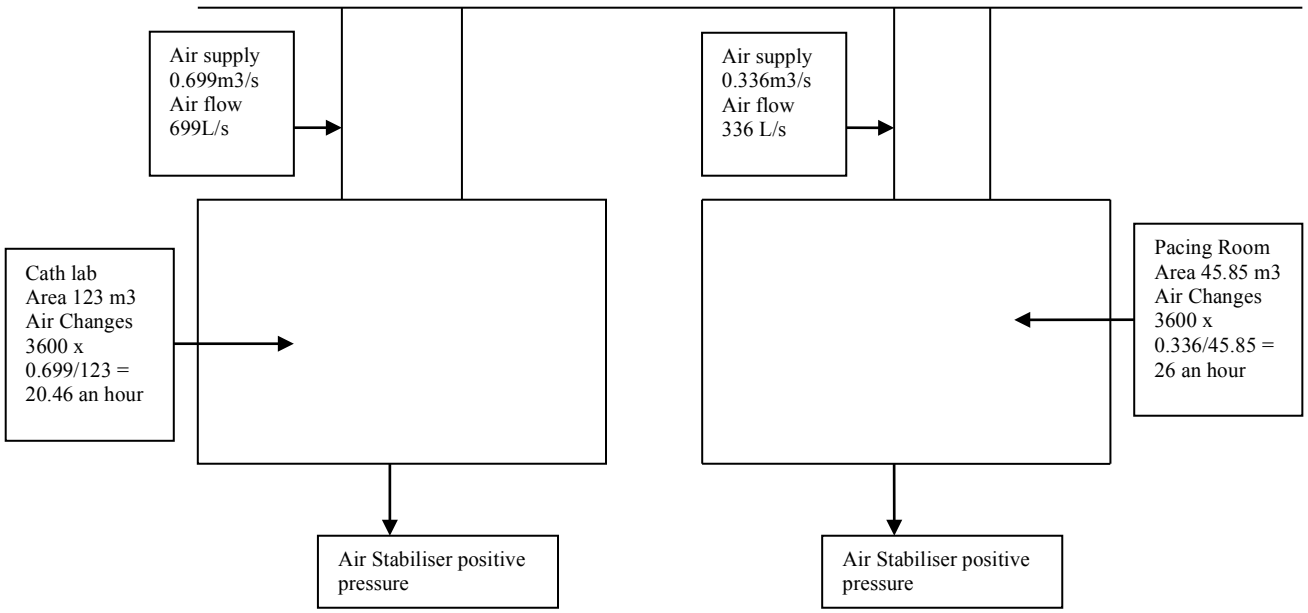
Air supply
0.699m3/s
Air flow
699L/s
Air supply
0.336m3/s
Air flow
336 L/s
Cath lab
Area 123 m3
Air Changes
3600 x
0.699/123 =
20.46 an hour
Pacing Room
Area 45.85 m3
Air Changes
3600 x
0.336/45.85 =
26 an hour
Air Stabiliser positive pressure
Air Stabiliser positive pressure